

Simultaneous Determination of Nicorandil in Pharmaceutical Dosage Form by HPLC Method

Emad Mahmoud Abd El-halim^{1*}, Mounir Zaki, Alaa Amin², Hanaa Khater³

¹Methodology section head, ADWIA Pharmaceutical Compan, 10th of Ramadan city-Egypt

²Benha University. Egypt

Available Online: 15th June, 2015

ABSTRACT

A rapid and accurate HPLC method was developed for determination of Nicorandil in tablet dosage form. The chromatographic separation was conducted on Agilent 1200 with DA detector; using BDS column ; ACE, (150 x 4.6 mm, 5 µm). The mobile phase was isocratic consisted of Methanol : Phosphate buffer in ratio of (30 : 70 v/v) (buffer is composed of 6.8 gm potassium dihydrogen phosphate per liter and was delivered to the system at a flow rate of 1 ml/min. An injection volume of 20 µl . The detection wavelength (λ_{max}) was 262 nm . All assays were performed at ambient conditions. The calibration curve in mobile phase was linear with correlation coefficient (r^2) = 0.99999; over a concentration range of 5 – 20 mcg/ ml with a retention time of 3.19 minutes. . The percentage recoveries of Nicorandil were 98.83% to 101.71% ; respectively. The relative standard deviation (RSD) was found to be 1.06% The proposed method was validated and successfully applied for simultaneous determination of Nicorandil in tablets. The method described is quite suitable for routine analysis of tablets and for their dissolution quantitation.

Keywords: Nicorandil; HPLC; BDS column; Method Validation.

INTRODUCTION

Nicorandil (NIC, N-[2-(nitroxy)ethyl]-3-pyridinecarboxamide) is a novel kind of compound in the treatment of angina. It possesses dual mechanism of action : as a potassium channel opener that causes vasodilation of arterioles and large coronary arteries and as nitrate compound that produces venous vasodilation through stimulation of granulate cyclase, which protects heart against hypoxia-induced apoptosis^{1,2}.

However, NIC is not chemically stable and its amide group and nitrate (ester) are easily dissociated, oxidized, reduced and displaced. Being kept at 60°C for 420 min, NIC produces 2-(3- pyridyl)-2- oxazoline, 2 aminoethyl nicotinate, HEN and NA at pH 4.0, 7.0 and 9.0³. Upon storage at room temperature NIC also produces NI , HEN and NA

In vivo , metabolites of NIC are HEN , N-methyl-nicotinamide, nicotinamide and NA⁴. The determination of NIC has been reported by many efficacious analytical methods, Such as HPLC, single-sweep oscillography , spectrophotometry , UV spectrophotometry etc⁵, at the same time, there are several techniques used Simultaneously determine NIC and one of its degradation products, such as NI by HPLC and HEN by HPLC , HPCE and HPTLC⁶⁻⁷

MATERIALS AND METHODS

Materials

All chemicals and reagents used were HPLC grade. Pure standards of Artemether were obtained from Hetero

Drugs, Hyderabad. Acetonitrile was HPLC grade from Romil chemicals. Water for chromatography was from Merck.

Nicorandil were obtained from Sinochem, China. Methanol and Potassium dihydrogen phosphate was HPLC grade from Fisher chemicals.

Methods

Analytical procedure for simultaneous determination of Nicorandil in tablet dissolution

Chromatographic condition: Agilent 1200 with DA detector was used. BDS column ; ACE, (150 x 4.6 mm, 5 µm) was used as a stationary phase. Mobile phase was isocratic consisted of Methanol : Phosphate buffer in ratio of (30 : 70 v/v) (buffer is composed of : 6.8 gm potassium dihydrogen phosphate per liter, delivered to the system at a flow rate of 1 ml/min, An injection volume of 20 µl was used The detection wavelength (λ_{max}) was 262 nm , run time was 5 minute. The column was maintained at ambient temperature.

Preparation of stock and working standard solution

Standard stock solution (10 µg/ml) of Nicorandil, were prepared separately in mobile phase. Working standard solutions were prepared and further diluted in mobile phase to contain a mixture of metformin hydrochloride and pioglitazone hydrochloride in over the linearity range from 5 - 20 µg/ml respectively.

Analytical method validation

Selectivity: It provides an indication of the selectivity and specificity of the procedure. The method is to be

selective, if the main peak is well resolved from any other peak by resolution of minimum 2

This could be done injecting placebo and compare it with that of standard and dissolution samples, then peak purity was ascertained by use of DAD

Linearity: is defined by the correlation coefficient, which should be found NLT 0.99, using peak area responses, Linearity for single point standardization should extend to at least 20% beyond the specification range and include the target Conc. This was performed by preparing 5 different concentrations, and then making 3 replicates of each concentration The linear working range were determined from the constructed standard calibration curve.

Intraday Precision: This study was conducted by performing multiple analyses on a suitable number of portions of a homogeneous sample.

This was performed by assaying multiple aliquots with the same concentration starting from the first step to the final step of analysis

The analytical precision of the method was determined by the relative standard deviation.

Inter-day Reproducibility (method ruggedness): the degree of reproducibility determined by analysis of samples from homogeneous lot of materials, under different but typical test conditions The method is to be rugged, at any item if the pooled %RSD of the total

number of replicates that have been made in this item is within the acceptance criteria, 3 replicates of a single sample of powder material are used for each determination. First day: 3 replicates, on a second day: 3 replicates, then on third day: 3 replicates of freshly prepared test from the same sample are analyzed, under the same conditions.

Accuracy and Recovery: Accuracy was evaluated by spiking standard solution. The measurements are made at a Conc. of Standard Mix which is found to be the target concentration, and at suitable intervals around this point The dissolution samples was spiked with known quantities of St. Using three determinations over five Concentrations level covering the specified range (i.e. five concentrations and three replicates).

Relative recoveries of all concentrations of Nicorandil used in the standards were evaluated by comparing their peak area with those obtained from the calibration curve equation

Specificity: The PDA chromatograms of the Nicorandil in standard and sample were recorded. In the chromatograms of the formulations, some additional peaks were observed which may be due to excipients present in the formulations. These peaks however did not interfere with the standard peaks, which demonstrate that the assay method is specific. Furthermore, the purity of the peaks was studied by peak purity studies. The results

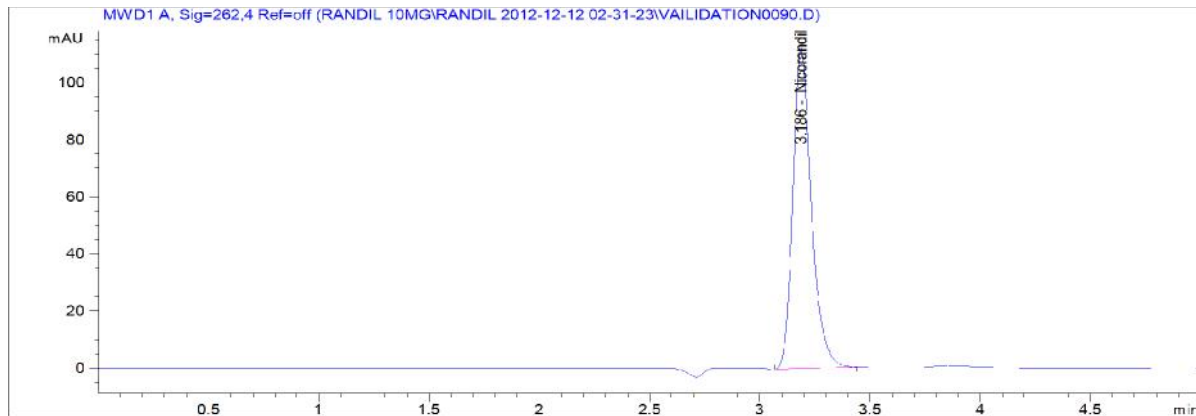


Figure 1: HPLC Chromatogram of Nicorandil

Linearity curve

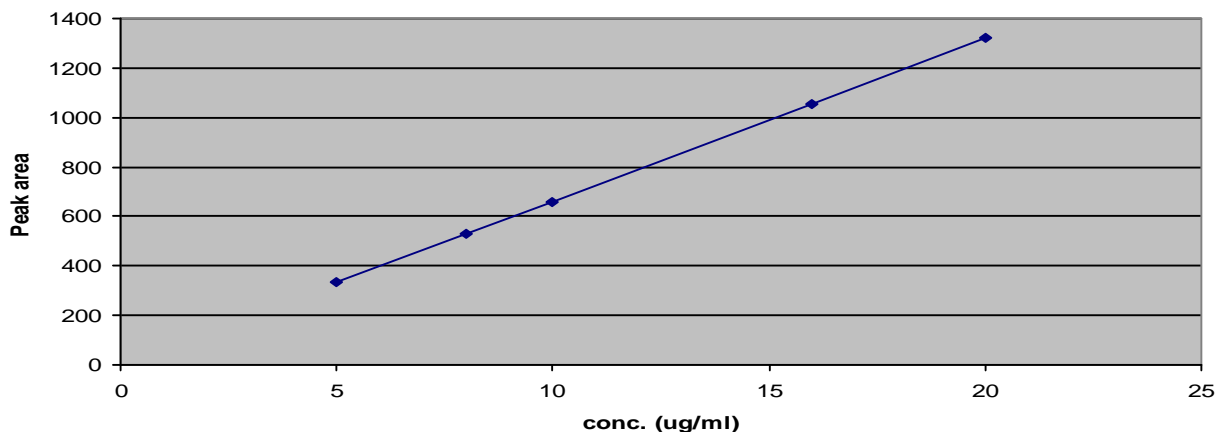


Figure 2: Calibration curve of Standard Nicorandil

revealed that the peak is free from interferences, which shows that the HPLC method is specific.

Linearity: The response for the detector was determined to be linear over the range of 5-20 µg/ml (5, 8, 10, 16 & 20) as shown in figure 2. Each of the concentrations was injected in triplicate to get reproducible response. The calibration curve was plotted as concentration of the respective drug versus the response at each level. The proposed method was evaluated by its correlation coefficient and intercept value calculated in the statistical study. They were represented by the linear regression equation

$$Y_{\text{Nicorandil}} = 660.6626 X - 360, r^2 = 0.9999$$

Slopes and intercepts were obtained by using regression equation ($Y = mx + c$) and least square treatment of the results used to confirm linearity of the method developed.

Quantification limit

The limit of detection (LOD) and limit of quantification (LOQ) of the developed method was determined by injecting progressively low concentrations of the standard solutions using the developed methods. The LOD is the lowest concentration of the analyte that can be detected with signal to noise ratio (3:1) and LOQ is the lowest concentration that can be quantified with acceptable precision and accuracy with signal to noise ratio (10:1). The LOD of Nicorandil found to be 0.35µg/ml respectively. The LOQ to be 1.07µg/ml respectively

Solution Stability

In this study, the mobile phase, the standard solutions, and the sample solution were subjected to long term (3 days) stability studies. The stability of these solutions was studied by performing the experiment and looking for changes in separation, retention, and asymmetry of the peaks which were then compared with the pattern of the chromatogram of freshly prepared solutions

System suitability

The resolution, capacity factor, theoretical plates/meter, Rt values and peak symmetry were calculated for the standard solutions. The values obtained demonstrated the suitability of the system for the analysis of the above drug combinations System suitability parameters might be fall within $\pm 3\%$ standard deviation range during routine performance of the method.

RESULTS AND DISCUSSION

The proposed HPLC method required fewer reagents and materials, and it is simple and less time consuming. This method could be used in quality control test in pharmaceutical industries.

Conclusion

This method is simple, specific and easy to perform and requires short time to analyze the samples. Low limit of quantification and limit of detection makes this method suitable for use in quality control. This method enables simultaneous determination of Nicorandil because of good separation and resolution of the chromatographic peaks. The method was found to be accurate, precise, linear, and rugged.

Acknowledgement

The authors are grateful to ADWIA Pharmaceutical Company (El Sharkia, Egypt) for her ultimate support for research and development team.

CONFLICT OF INTEREST

Authors declare that they have no conflict of interest

REFERENCES

1. Bachert EL, Fung HL: High-performance liquid chromatographic method for stability and pharmacokinetic studies of nicorandil. *J Chromatogr* (1993); 619(2):336-341
2. Ojha A, Pargal A.: Determination of nicorandil concentrations in human plasma using liquid chromatography. *J Pharm Biomed Anal* (1999); 21(1):175-178.
3. Ishizaki T, Chiba K, Sugauma T, Sasaki T, Kamiyama H, Nakano H: Pharmacokinetics of nicorandil, a new coronary vasodilator, in dogs. *J Pharm Sci* (1984); 73(4):494-498.
4. Andresek S, Smidovnik A, Pecavar A, Prosek M.: Routine and sensitive method for determination of nicorandil in human plasma developed for liquid chromatography with ultraviolet and mass spectrometric detection. *J Chromatogr B Biomed Sci App* (1999); 735(1):103-109.
5. Tipre DN, Vavia PR. :Formulation optimization and stability study of transdermal therapeutic system of nicorandil. *Pharm Dev Technol* (1984); 7(3):325-332.
6. Schwende FJ, Lewis RC: Determination of nicorandil in plasma using high-performance liquid chromatography with photoconductivity and ultraviolet detection : Application to pre-clinical pharmacokinetics in beagle dogs .*J. Chromatogr. Biomed. Appl* (1990); (525) :151-160.
7. Tanikawa M, Uzu M, Ohsawa Y, Fukushima M: Sensitive method for determination of nicorandil in human plasma by reversed-phase high-performance liquid chromatography with ultraviolet detection. *J. Chromatogr. Biomed. Appl* (1993); 617 (1): 163-167.