

# Overview of Machine Learning and AI Algorithms is Being Integrated into Coronary Artery Calcium Scoring

Shipra Saroj<sup>1\*</sup>, Sohel Rana<sup>2</sup>, Kanika Kiran<sup>3</sup>, Rufaida Binte Jalal<sup>4</sup>, Pallavi Sharma<sup>5</sup>, Palvi Thakur<sup>6</sup>, Lalit Kumar Gupta<sup>7</sup>

<sup>1\*</sup>Assistant Professor, Department of Radiological Imaging Techniques, Rayat Bahra University, Kharar, Punjab, India.  
Email: [shiprasaraj789@gmail.com](mailto:shiprasaraj789@gmail.com) (Corresponding Author)

<sup>2</sup>Assistant Professor, Department of Radiological Imaging Techniques, Midnapore City College, West Bengal, India

<sup>3</sup>Assistant Professor, Department of Radiological Imaging Techniques, Rayat Bahra University, Kharar, Punjab, India

<sup>4</sup>Assistant Professor, Department of Radiological Imaging Techniques, Rayat Bahra University, Kharar, Punjab, India

<sup>5</sup>Assistant Professor, Department of Radiological Imaging Techniques, Saraswati College of Pharmacy, SGC Group, Gharuan, Mohali, Punjab, India

<sup>6</sup>Assistant Professor, Department of Microbiology, Swami Vivekanand Institute of Engineering and Technology, Banur, India

<sup>7</sup>Professor, Department of Radiology, Rayat Bahra University, Kharar, Punjab, India

## Abstract

Coronary Artery Calcium Scoring (CACS), using the Agatston score in particular, is commonly utilized in early detection and assessment of coronary artery disease (CAD). ECG-gated CT scans have historically complemented the procedure using technologies such as EBCT, MDCT, and DSCT. Although effective, these methods are challenged by accuracy and efficiency. Techniques have been revolutionized with advancements in artificial intelligence (AI), especially with deep learning techniques such as convolutional neural networks (CNNs). These technologies now make it possible to conduct fully automated calcium scoring from gated and non-gated CT scans with increased speed and accuracy. AI also makes it possible to derive complex imaging characteristics, including lesion location and density, improving cardiovascular risk prediction. New models integrating clinical, anatomical, and imaging data are assisting in making more personalized treatment plans. Yet, challenges like data unpredictability, limited clarity of AI algorithms, and data privacy and fairness issues persist. In spite of that, AI incorporation represents a significant leap in cardiovascular imaging, with ongoing exploration and regulation essential for safety and efficacy in clinical practice.

**Keywords:** Coronary Artery disease; cardiovascular disease; Artificial intelligence; Deep learning; Multidetector Computed Tomography; Electron Beam Computed Tomography

**How to cite this article:** Saroj S, Rana S, Kiran K, Jalal RB, Sharma P, Thakur P, Gupta LK. Overview of Machine Learning and AI Algorithms is Being Integrated into Coronary Artery Calcium Scoring. *Int J Drug Deliv Technol.* 2026;16(13s): 658-670. DOI: 10.25258/ijddt.16.13s.73

## INTRODUCTION

In specialized CT imaging, coronary artery calcium (CAC) scoring is frequently employed to determine coronary atherosclerotic plaque load and predict cardiovascular disease risk (CVD). (van Velzen et al., 2020). This is one of the best-studied and most available diagnostics in cardiovascular medicine. (Greenland et al., 2018). Since intravenous contrast is not required, CAC is generally assessed noninvasively with the use of electrocardiogram-gated computed tomography (CT) imaging of the heart. Hecht HS et al., 2015). Calcium deposits in the coronary arteries, an indication of vascular calcification and burden of atherosclerotic plaque, are measured in CAC scoring. The progression of Coronary Artery Calcium types is depicted in Figure 1 (Quddus R et al., 2024). Acute coronary syndrome (ACS), myocardial infarction (MI), and even life-

threatening coronary thrombosis may be triggered by the breaking or erosion of plaques with time (Nguyen AM et al., 2024). In a 15-year follow-up study in recent times, the mortality among patients with zero CAC was very low and increased progressively with increasing risk classes of CAC scores (1–99, 100–399, and > 400) (Gräni et al., 2018). The Society of Thoracic Radiology (STR) and the Society of Cardiovascular Computed Tomography (SCCT) have now included coronary artery calcium (CAC) scanning in their guidelines and appropriateness criteria for atherosclerotic cardiovascular disease (ASCVD) risk assessment in asymptomatic individuals (Hecht et al., 2018; Greenland et al., 2010). Numerous studies reveal a dose-response relationship between rising CAD burden and cardiovascular risk, and the lack of CAD on CCTA indicates low incidence for cardiovascular events

\*Author for Correspondence: [shiprasaraj789@gmail.com](mailto:shiprasaraj789@gmail.com)

(Al'Aref et al., 2019; Budoff et al., 2008; Miller et al., 2008). The American Heart Association (AHA), American College of Cardiology (ACC), and European Society of Cardiology (ESC) each have practice guidelines for the management of stable angina chest pain that support the use of CCTA as a first or second-line diagnostic tool in symptomatic patients presenting with suspected obstructive CAD (Al'Aref et al., 2019; Cho I et al., 2015; Lin FY et al., 2010). But in everyday clinical practice, a substantial majority of patients who received CCTA had minimal or no CAD (Al'Aref et al., 2019; Montalescot G et al., 2013; Fihn SD et al., 2012). In contrast to traditional work-ups with stress testing, coronary CTA enables rapid assessment of patients, with reduced time to diagnosis and discharge. 1 through 3 The high negative predictive value for excluding severe coronary stenosis and ACS is the key benefit of coronary CTA (Ferencik et al., 2019). The three CAC scoring methods are the Agatston score, volume score, and mass score (Table 1).

Among them, the Agatston method is most popular and accepted as the gold standard. In regard to the whole area and the maximum calcification attenuation, the Agatston score is a weighted summation of calcified plaques (Gupta, A et al., 2022). Artificial intelligence (AI) provides unique advantages in coronary artery calcium score (CACS) and cardiovascular disease (CVD) risk prediction, with its use in medicine and radiology increasing. AI can potentially extract quantitative CACS from standard chest CT protocols that are not specifically intended for this, including cardiac CT angiography (CCTA), low-dose CT (LDCT), and positron emission tomography (PET)/CT attenuation scans. AI can also upgrade the time-consuming, tedious, and labor-intensive tasks of calcium segmentation and quantification (Aromiwura AA et al., 2024).

## 1. Traditional CAC Scoring Methods:-

### 1.1. Agatston Score (AS)

In clinical practice, the most widely used scoring system is the AS. The first suggestion was made by Warren Janowitz and Arthur Agatston in 1990. The AS is acquired with electron beam (EB) CT with a  $512 \times 512$  reconstruction matrix, 3-mm slice thickness, 130-KVp tube voltage, and 630mAs tube current. A 3-mm slice thickness, variable mA based on patient body weight, and 120 kVp have been used to convert the score to multidetector CT (MDCT). The rating considers both the peak coronary calcific density and total area, and is obtained by summing the rating of all the calcified lesions (Figures 2 and 3). Lesions with an area  $\geq 1 \text{ mm}^2$  and CT attenuation  $> 130$  Hounsfield units (HU) are excluded to avoid image noise (Figure 4). A density

weighting factor (DWF) is used to multiply the lesion area to calculate the individual lesion score. A maximal CT attenuation value of a given calcified plaque is applied to derive the DWF (DWF: 130 to 199 HU = 1; 200 to 299 HU = 2; 300 to 399 HU = 3; and  $\geq 400$  HU = 4).  $AS(\text{lesion}) = \text{Area} \times \text{DWF}$  (9) In order to determine the overall AS, individual scores—irrespective of location or distribution—are then added up.  $AS(\text{total}) = \sum AS(\text{lesion})$  (Kumar P et al., 2023). The CAC score enables collaborative decision-making in symptom-free individuals. Following Agatston CAC grading, increased CAC measurements can be used as an additional "biomarker" to improve risk prediction in patients with intermediate CAC values (Top). Identification of high-risk cases for the most aggressive preventive therapy would be a principal role, although some patients would be reclassified downward. Instead, using advanced CAC measures, an entirely new CAC score could be constructed, perhaps enhancing risk prediction in all patients (Bottom) (Figure 5). (Blaha, M.J. et al., 2017).

### 1.2. Fundamental framework for building a new CAC score

It is necessary to step back and examine fundamental questions about the nature of the CAC score and consider how to refine it. To inform and frame the development of a new scoring system, answers to these questions are essential. First, why does CAC scoring predict coronary risk so well? This topic is addressed by advances in our understanding of the relationship between atherosclerosis and acute coronary events. Whereas the scientific community once was interested in identifying occult obstructive coronary disease, we now understand that the most sensitive predictor of future events in asymptomatic individuals is the total burden of atherosclerosis and not lumen stenosis. For it to be most effective, a new score must be equally easy to play and read quickly.

More precisely, a new CAC score must be at least as repeatable as the Agatston score in terms of observer and scan variability. A new CAC score should ideally be qualitatively reproducible on non-gated chest CT scans. The Society of Cardiovascular Computed Tomography and the Society of Thoracic Radiology have published a new recommendation statement advocating for at least qualitative CAC scoring on all nongated chest CT scans, in response to mounting evidence regarding the value of qualitative CAC scoring on lung cancer screening studies. (Blaha MJ et al., 2017; Hecht HS et al., 2017). The effect of including the number of lesions, max HU, distance-based and territories, and distribution of CAC along territories (diffusivity) in addition to the mass score model was tested, and the effect of mass scores

was tested using multivariable Cox models. Cox modeling, which is a machine learning method, provides interpretable results that are able to account for the effect of image features that deep learning cannot. All of the Cox models in our investigation were trained and evaluated using the same data in order to improve comparability. (Hoori A et al., 2024).

## 2. Artificial Intelligence in Medical Imaging

In recent years, the use of artificial intelligence (AI) techniques in radiology has increased dramatically in a number of fields, including cardiac imaging. (Rogers, et al., 2019; Lim et al., 2020).

Furthermore, the potential of AI in medical imaging to transform clinical practice by facilitating picture acquisition and interpretation, improving image quality, and disease detection has generated a lot of enthusiasm. (Rubin et al., 2019). The AI application has also been shown to improve risk stratification and prediction across a broad array of disciplines and disease phases (Table 2). Using artificial intelligence in cardiovascular imaging via "radiomics" would enhance disease diagnosis and, ultimately, prognosis. All imaging modalities have embraced AI, with it now being used for autonomous measurements and image segmentation, such as the autonomous assessment of coronary artery calcium (CAC). (Abdelrahman et al., 2024). As a helpful add-on tool in clinical use, artificial intelligence (AI) is increasingly being used in diagnostic medicine and radiology to deliver objective and reproducible diagnoses by extracting relevant features from medical imaging information and applying them to classifiers for the automated identification of cardiovascular disease. A type of artificial intelligence referred to as machine learning, or in some cases as deep learning, employs algorithms to merge extensive amounts of data, such as clinical data and coronary anatomical features, to forecast cardiac events as precisely as possible. (Wang W et al., 2019). Through enhanced image generation and more precise diagnoses, artificial intelligence (AI), particularly via machine learning (ML) techniques such as convolutional neural networks (CNNs), has the ability to revolutionize cardiac CT entirely. These AI-based technologies have the capability to significantly streamline the imaging process, allowing radiologists to have increased time to work and deliver results. This acceleration of workflow is important as it allows doctors to initiate patient interventions earlier on, which can have improved outcomes. (ToluAkinnowo OZ et al., 2025).

## 3. Deep learning in Medical Imaging

A fully automatic branch-level CAC scoring algorithm using DL and involving the left main (LM), left anterior

descending (LAD), circumflex (CX), and right coronary artery (RCA) regions was available and tested. The goal was to assess whether the total Agatston scores of the automated model were well correlated with the manual Agatston scoring and whether the vessel labels it provided were concordant with human readers. (David J Winkel et al., 2022). To evaluate whether an automated CACS detector that allows CT calcium score imaging quantification can have an equivalent risk prediction for cardiac risk stratification with a similar degree of convenience to manual measurement, the present study was undertaken. (Wang W et al., 2019).

An aggregation of DL methods integrates a variety of models to enhance the functionality of CAC detection systems. Bagging, boosting, and stacking are some methods that enhance robustness in complex or uncertain situations through counterbalancing the limitations of individual models. (Vivekanandan DD et al., 2024).

### 3.1. Algorithmic Analysis

The obtained signals were subjected to sophisticated algorithms for anomaly identification and pattern recognition, such as machine learning models and signal processing techniques. (Rana N et al., 2025).

### 3.2. Outcome Prediction

Most imaging markers of cardiovascular risk, such as radiomics, body fat, plaque morphology, and CAC score, are being integrated into traditional clinical risk factors to develop prediction models that will improve the performance of current risk scores and prognostic tools. AI plays a key role in this process because it enables the combination of imaging and clinical data, as well as the inclusion of additional clinical factors. Several fusion models that merge multiple resources have been developed and effectively used for detecting acute CVD, phenotyping CVD, and assessing CVD risk and severity. (Onnis C et al., 2024).

## 4. Ethics, Limitations, and Standards of Artificial Intelligence in CAD Imaging

The ease with which machine learning can access data may lead to ethical issues. Big data analysis can be completed in minutes, raising concerns about proper consent and secure PHI storage. For physicians wanting to incorporate these practices, the "black box" nature of AI might cause confusion. To prevent biased outcomes and unintended extrapolation, clinicians need to understand AI's limitations and specific validation (Covas P et al., 2022).

## 5. Objectives And Scope of the Review

The CACS was postulated by Agatston et al. in 1990, who provided essential information on the ability of (electron-beam) CT to measure CAC. Irrespective of the tremendous technological breakthroughs in CT scanners over the years since then, the longevity of CACS was ensured by the beauty and simplicity of the proposed method. The Agatston score is a radiological entity derived from non-contrast, 3 mm electrocardiogram-gated (ECG-gated) images. It employs a semiautomated calcified plaque quantification based on 1 mm<sup>2</sup> and 130 Hounsfield Units (HU) as the lowest cutoffs to differentiate calcified plaques from noise. The weighted sum score of the peak density multiplied by the area of the plaque, summed across all qualifying lesions, is the Agatston score. (Gennari AG et al., 2024).

### 5.1. Image requirements

The spatial resolution and contrast-to-noise ratio (CNR) of CT images should be superb for AI analysis. Reducing the radiation exposure has to be balanced with this requirement. Current routine CT scanning is already employing new deep-learning image reconstruction methods, which can aid in this direction. Still, radiation levels and image reconstruction methods need to be manipulated. This may mean that various types of CT imaging could be successfully processed, and the image type is not the most important factor. (Yamaoka T et al., 2023)

## 6. TRADITIONAL METHODS OF CAC SCORING

### 6.1. Non-gated chest CT model: internal validation

For the Stanford test set, there was almost perfect agreement (Kappa = 0.84,  $P < 0.0001$ ) when the CAC scores automatically and manually derived were compared with each other using Cohen's Kappa statistic. In the MESA test set, there was moderate agreement (Kappa = 0.52,  $P < 0.0001$ ) (Fig. 6). As per current cholesterol recommendations, the statin drug must be initiated once the CAC score is  $\geq 100$  in an attempt to reduce the risk of future CVD events. Positive predictive values and sensitivity were exhibited by the non-gated model for binary classification of patients with CAC scores  $\geq 100$ . (Eng D et al., 2021).

### 6.2. Non-gated chest CT model: external validation

The non-gated model was externally validated with data from four sites. Substantial agreement existed at site 1 (Kappa = 0.80,  $P < 0.0001$ ), fair agreement at sites 2 and 3 (Kappa = 0.68 and 0.64, respectively;  $P < 0.0001$ ), and fair agreement at site 4 (Kappa = 0.58,  $P < 0.0001$ ) when bucketed CAC values were compared using Cohen's Kappa statistic. At all sites, the diagnostic accuracy for

detecting any CAC ( $\geq 1$ ) was excellent (sensitivity range: 82–94% and PPV range: 87–100%). The greatest sensitivity and PPV for detecting CAC  $\geq 100$  were found at Sites 1 and 2.

(Eng D et al., 2021).

## 7. Electron Beam Computed Tomography (EBCT).

It became known during the 1960s that the pathophysiology behind the development of atherosclerotic plaque was associated with calcium deposition within the coronary arteries. It also became known that fluoroscopy could be utilized in order to visualize calcification. In a groundbreaking study of coronary calcium quantitation, Agatston et al. (1990, researchers identified regions of high attenuation in the heart on EBCT images shortly after the technology had been invented. A calcium score was generated by EBCT-measured coronary calcification in 88 subjects based on the number, area, and attenuation of calcifications. The authors only sought to illustrate that EBCT was better than fluoroscopy for detecting calcification; the predictive value of the calcium score was still uncertain. (Kulkarni et al., 2021). EBCT employs a fixed source/detector assembly in which a rotating electron beam is scanned back and forth across a series of one to four semicircular tungsten targets to generate X-rays.

It is also known as ultrafast computed tomography (CT) (Imatron C-100, C-150) and cine-CT. The imaging chain contains no moving parts, so scanning can be performed in rapid succession over the cardiac cycle or at specified times. (Rumberger JA et al., 1997). The whole heart may be scanned during one or two short breath holds. Standardized methods are now available for employing EBCT to scan, detect, and quantify coronary artery calcium. (Rumberger et al., 1999). Coronary artery calcium is detected by executing sequential, single-slice, 3-mm-thick, 100-ms scans. During as many cardiac cycles as possible, 40 successive heart tomograms synchronized with the heart rate during late diastole can be obtained using this "high resolution" volume scanning mode. Two successive breath holds may be required to obtain scans from the origin of the aorta and the left main coronary artery origin through distal right coronary artery sections, depending on the pulse rate. When the field of view is 300 mm, the in-plane spatial resolution is 0.4 mm<sup>2</sup>. Coronary artery calcium can be identified without an intravenous contrast injection because the calcification of the arterial walls exhibits comparatively high Hounsfield (H) densities, which are two to ten times higher than those of the surrounding soft tissue. Since high-density intramural coronary calcium deposits lie adjacent to low-density soft tissue and pericardiac fat, it is fairly simple to visually discern calcium to determine the calcium burden of the coronary

arteries using EBCT (Rumberger JA et al., 1997). EBCT possesses minimal motion artifacts and superb temporal resolution and is therefore ideal for imaging fast-moving objects such as the beating heart.

### **8. Dual Source Computed Tomography (DSCT)**

The DSCT system being tested has two X-ray tubes and two corresponding detectors. The two acquisition systems are mounted with a 90° angular offset on the rotating gantry. Because of the limited space available on the gantry, one detector (A) scans the entire scan field of view (50 cm in diameter), and the other detector (B) scans a smaller central field of view (26 cm in diameter). (Fig. 7). ( Flohr TG et al., 2006). We looked at two methods of combining CTCA and CS. First, we discovered whether a low CS could be applied to exclude significant coronary artery stenoses misinterpreted by CTCA, and whether a high CS could be applied to detect stenoses that CTCA missed. (Leschka, S et al., 2015).

### **9. Multidetector Computed Tomography (MDCT)**

Increased x-ray tube rotation speed (from 1 sec/rotation to 0.5 sec/rotation) and tube rotation speed number of detectors are the key technological advances of MDCT. Detectors are stacked on the patient's long axis (the z-axis) in MDCT use, and with every rotation of the x-ray tube, four to sixteen CT slices can be collected. Detectors run in alignment along the axial plane of the patient (the X-axis) in standard CT scanners. Multichannel helical CT and multidetector-row CT are synonyms. MDCT design in the majority of instances reduces scanning time to less than one minute and greatly expands volume covered. In conventional CT, electrical cables run through detectors and the x-ray tube, restricting them from rotating more than 180 degrees. MDCT, however, does not have electrical cords within the gantry due to its slide ring technology. These metal conducting rings avoid cable twisting and allow unbroken high-speed rotation of the X-ray tube and detector array. (El-Khoury GY et al., 2004). Though MDCT emits more radiation dosage than EBCT, it is used to enhance spatial resolution and allow 3D reconstruction of coronary anatomy.

### **10. Clinical Applications and Real-World Deployments**

The ability of a clinical test to first recognize an illness and subsequently assist in implementing measures that influence the natural course of the disease and improve outcomes characterizes its value. Coronary artery calcium is special in that it can be visualized by CT and also is a risk factor for CAD (George A et al.,2008). Wang et al. studied a patient cohort with no CAD

diagnosis in the Multi-Ethnic study of Atherosclerosis (MESA) study. Myocardial blood flow was measured through MRI at rest and hyperemia induced by adenosine, and multi-detector CT was employed to calculate the Agatston scores for coronary calcification. The research proved that myocardial perfusion reserve in asymptomatic individuals was inversely related to the severity and presence of CAC irrespective of the presence of CAD risk factors (Wang L et al., 2006).

### **11. Future Directions and Challenges**

This approach may determine the most appropriate individuals for CAC scoring, thus alleviating concerns regarding radiation exposure and healthcare costs. Furthermore, advancements in risk assessment algorithms and imaging technology are likely to enhance the accuracy and applicability of CAC scoring across various patient populations. These advancements could enhance the reliability of CAC score results and promote its application as a cardiovascular risk assessment tool. Enabling the integration of CAC scoring into routine clinical practice involves intercooperation from all stakeholders, such as clinicians, researchers, and lawmakers (Majhi L et al., 2022).

### **Conclusion**

Coronary Artery Calcium Scoring (CACS), particularly via the Agatston method, remains a key noninvasive tool for evaluating coronary atherosclerotic burden and cardiovascular risk. Traditional imaging techniques such as EBCT, MDCT, and DSCT have supported accurate calcium quantification. However, limitations exist in precision and applicability, especially for intermediate-risk individuals. Artificial intelligence (AI), including machine learning (ML) and deep learning (DL) methods like convolutional neural networks (CNNs), is revolutionizing CACS by enabling automated, reproducible scoring from both gated and non-gated CT scans. These innovations enhance workflow efficiency and facilitate the extraction of advanced imaging features, improving risk prediction. Notwithstanding these advances, ethical and regulatory considerations—such as data security and model transparency—must be addressed. Ultimately, integrating AI into CACS presents a promising step toward more personalized, efficient, and accurate cardiovascular risk assessment, provided rigorous validation and multidisciplinary collaboration continue.

### **Additional information**

**Source of funding-** N/A

**Conflict of interest-** N/A

### Authors involvement-

**Shipra Saroj** conceptualized the review topic, led the literature search, wrote the section on artificial intelligence, and wrote the initial draft of the manuscript.

**Sohel Rana** contributed to data extraction and thematic organization of the review.

### Acknowledgements

I sincerely acknowledge **Dr. Lalit Kumar Gupta** for his invaluable guidance, insightful feedback, and constant encouragement throughout this study. I extend my gratitude to the study participants for their cooperation and to my family for their unwavering support. Special thanks to **Mr. Sohel Rana** for his kind encouragement during challenging times. Above all, I am grateful to the Almighty for the strength and wisdom to complete this work.

### Reference

- van Velzen, S. G., Lessmann, N., Velthuis, B. K., Bank, I. E., van den Bongard, D. H., Leiner, T., ... & Išgum, I. (2020). Deep learning for automatic calcium scoring in CT: validation using multiple cardiac CT and chest CT protocols. *Radiology*, 295(1), 66-79. <https://doi.org/10.1148/radiol.2020191621>
- Gräni, C., Vontobel, J., Benz, D. C., Bacanovic, S., Giannopoulos, A. A., Messerli, M., ... Buechel, R. R. (2018). Ultra-low-dose coronary artery calcium scoring using novel scoring thresholds for low tube voltage protocols—a pilot study. *European Heart Journal - Cardiovascular Imaging*. <https://doi.org/10.1093/ehjci/jev019>
- Hecht HS (2015) Coronary artery calcium scanning: past, present, and future. *JACC Cardiovasc Imaging* 8:579–596.
- Quddus R. Enhancing Cardiovascular Risk Assessment with Coronary Artery Calcium Scoring: A Comprehensive Study.2024
- Nguyen AM, Liu J, Mathai TS, Grayson PC, Summers RM. Automated plaque detection and Agatston score estimation on non-contrast CT scans: a multicenter study. ArXiv. 2024 Feb 14:arXiv-2402.
- Hecht, H. S., Blaha, M. J., Kazerooni, E. A., Cury, R. C., Budoff, M., Leipsic, J., & Shaw, L. (2018). *CAC-DRS: Coronary Artery Calcium Data and Reporting System. An expert consensus document of the Society of Cardiovascular Computed Tomography (SCCT)*. *Journal of Cardiovascular Computed Tomography*, 12(3), 185-191. <https://doi.org/10.1016/j.jcct.2018.03.008>
- Greenland, P., Alpert, J. S., Beller, G. A., Benjamin, E. J., Budoff, M. J., Fayad, Z. A., ... Wenger, N. K. (2010). *2010 ACCF/AHA Guideline for Assessment of Cardiovascular Risk in Asymptomatic Adults*. *Journal of the American College of Cardiology*, 56(25), e50–e103. <https://doi.org/10.1016/j.jacc.2010.09.001>
- Greenland, P., Blaha, M. J., Budoff, M. J., Erbel, R., & Watson, K. E. (2018). Coronary calcium score and cardiovascular risk. *Journal of the American College of Cardiology*, 72(4), 434-447. <https://doi.org/10.1016/j.jacc.2018.05.027>
- Budoff MJ, Dowe D, Jollis JG, Gitter M, Sutherland J, Halamert E, Scherer M, Bellinger R, Martin A, Benton R, Delago A, Min JK. Diagnostic performance of 64-multidetector row coronary computed tomographic angiography for evaluation of coronary artery stenosis in individuals without known coronary artery disease: results from the prospective multicenter ACCURACY (Assessment by Coronary Computed Tomographic Angiography of Individuals Undergoing Invasive Coronary Angiography) trial. *J Am Coll Cardiol* 2008;52:1724–1732. <https://doi.org/10.1093/eurheartj/ehu358>
- Al'Aref, S. J., Maliakal, G., Singh, G., van Rosendael, A. R., Ma, X., Xu, Z., ... Shaw, L. J. (2019). *Machine learning of clinical variables and coronary artery calcium scoring for the prediction of obstructive coronary artery disease on coronary computed tomography angiography: analysis from the CONFIRM registry*. *European Heart Journal*. <https://doi.org/10.1093/eurheartj/ehz565>
- Miller JM, Rochitte CE, Dewey M, Arbab-Zadeh A, Niinuma H, Gottlieb I, Paul N, Clouse ME, Shapiro EP, Hoe J, Lardo AC, Bush DE, de Roos A, Cox C, Brinker J, Lima JA. Diagnostic performance of coronary angiography by 64-row CT. *N Engl J Med* 2008;359:2324–2336. <https://doi.org/10.1016/j.jacc.2010.11.078>
- Cho I, Chang HJ, O' Hartaigh B, Shin S, Sung JM, Lin FY, Achenbach S, Heo R, Berman DS, Budoff MJ, Callister TQ, Al-Mallah MH, Cademartiri F, Chinnaiyan K, Chow BJ, Dunning AM, DeLago A, Villines TC, Hadamitzky M, Hausleiter J, Leipsic J, Shaw LJ, Kaufmann PA, Cury RC, Feuchtner G, Kim YJ, Maffei E, Raff G, Pontone G, Andreini D, Min JK. Incremental prognostic utility of coronary CT angiography for asymptomatic patients based upon extent and severity of coronary artery calcium: results from the COronary CT Angiography Evaluation For Clinical Outcomes International Multicenter (CONFIRM) study. *Eur Heart J* 2015;36:501–508. <https://doi.org/10.1093/eurheartj/ehz296>
- Lin FY, Shaw LJ, Dunning AM, Labounty TM, Choi JH, Weinsaft JW, Koduru S, Gomez MJ, Delago AJ, Callister TQ, Berman DS, Min JK. Mortality risk in symptomatic patients with nonobstructive coronary

- artery disease: a prospective 2-center study of 2,583 patients undergoing 64-detector row coronary computed tomographic angiography. *J Am Coll Cardiol* 2011;58:510–519. <https://doi.org/10.1016/j.jacc.2010.11.078>
20. Montalescot G, Sechtem U, Achenbach S, Andreotti F, Arden C, Budaj A, Bugiardini R, Crea F, Cuisset T, Di Mario C, Ferreira JR, Gersh BJ, Gitt AK, Hulot JS, Marx N, Opie LH, Pfisterer M, Prescott E, Ruschitzka F, Sabate M, Senior R, Taggart DP, van der Wall EE, Vrints CJ, ESC Committee for Practice Guidelines, Zamorano JL, Achenbach S, Baumgartner H, Bax JJ, Bueno H, Dean V, Deaton C, Erol C, Fagard R, Ferrari R, Hasdai D, Hoes AW, Kirchhof P,
  21. Knuuti J, Kolh P, Lancellotti P, Linhart A, Nihoyannopoulos P, Piepoli MF, Ponikowski P,
  22. Sirnes PA, Tamargo JL, Tendera M, Torbicki A, Wijns W, Windecker S, Document Reviewers, Knuuti J, Valgimigli M, Bueno H, Claeys MJ, Donner-Banzhoff N, Erol C, Frank H, Funck-Brentano C, Gaemperli O, Gonzalez-Juanatey JR, HAMILIOS M, Hasdai D, Husted S, James SK, Kervinen K, Kolh P, Kristensen SD, Lancellotti P, Maggioni AP, Piepoli MF, Pries AR, Romeo F, Ryde n L, Simoons-Sel A, Sirnes PA, Steg PG, Timmis A, Wijns W, Windecker S, Yildirim A, Zamorano JL. 2013 ESC guidelines on the management of stable coronary artery disease: the
  23. Task Force on the management of stable coronary artery disease of the European Society of Cardiology. *Eur Heart J* 2013;34:2949–3003. <https://doi.org/10.1016/j.jcmg.2015.06.016>
  24. Fihn SD, Gardin JM, Abrams J, Berra K, Blankenship JC, Dallas AP, Douglas PS, Fody JM, Gerber TC, Hinderliter AL, King SB 3rd, Kligfield PD, Krumholz HM, Kwong RY, Lim MJ, Linderbaum JA, Mack MJ, Munger MA, Prager RL, Sabik JF, Shaw LJ, Sikkema JD, Smith CR Jr, Smith SC Jr, Spertus JA, Williams SV. 2012
  25. ACCF/AHA/ACP/AATS/PCNA/SCAI/STS Guideline for the diagnosis and management of patients with stable ischemic heart disease: a report of the American College of Cardiology Foundation/American Heart Association Task Force on Practice Guidelines, and the American College of Physicians, American Association for Thoracic Surgery, Preventive Cardiovascular Nurses Association, Society for Cardiovascular Angiography and Interventions, and Society of
  26. Thoracic Surgeons. *J Am Coll Cardiol* 2012;60:e44–e164. <https://doi.org/10.1038/s41598018-27347-8>
  27. Ferencik, M., Lu, M. T., Mayrhofer, T., Puchner, S. B., Liu, T., Maurovich-Horvat, P., ... Hoffmann, U. (2019). *Non-invasive fractional flow reserve derived from coronary computed tomography angiography in patients with acute chest pain: Subgroup analysis of the ROMICAT II trial. Journal of Cardiovascular Computed Tomography*. <https://doi.org/10.1016/j.jcct.2019.05.009>
  28. Gupta, A., Bera, K., Kikano, E., Pierce, J. D., Gan, J., Rajdev, M., ... & Gilkeson, R. C. (2022). Coronary artery calcium scoring: current status and future directions. *Radiographics*, 42(4), 947-967. <https://doi.org/10.1148/rg.210122>
  29. Aromi-wura AA, Kalra DK. Artificial intelligence in coronary artery calcium scoring. *Journal of Clinical Medicine*. 2024 Jun 13;13(12):3453. <https://doi.org/10.3390/jcm13123453>
  30. Kumar P, Bhatia M. Coronary Artery Calcium Data and Reporting System (CAC-DRS): A Primer. *J Cardiovasc Imaging*. 2023 Jan;31(1):1-17. <https://doi.org/10.4250/jcvi.2022.0029>
  31. Wang L, Jerosch-Herold M, Jacobs DR, Shahar E, Detrano R, Folsom AR, MESA Study Investigators. Coronary artery calcification and myocardial perfusion in asymptomatic adults: the MESA (Multi-Ethnic Study of Atherosclerosis). *Journal of the American College of Cardiology*. 2006 Sep 5;48(5):1018-26. <https://doi.org/10.1016/j.jcmg.2017.05.007>
  32. Blaha MJ, Mortensen MB, Kianoush S, Tota-Maharaj R, Cainzos-Achirica M. Coronary artery calcium scoring: is it time for a change in methodology?. *JACC: Cardiovascular Imaging*. 2017 Aug;10(8):923-37. <https://doi.org/10.1016/j.jcmg.2017.05.007>
  33. Hecht HS, Cronin P, Blaha MJ, Budoff MJ, Kazerooni EA, Narula J, Yankelevitz D, Abbara S. 2016 SCCT/STR guidelines for coronary artery calcium scoring of noncontrast noncardiac chest CT scans: a report of the Society of Cardiovascular Computed Tomography and Society of Thoracic Radiology. *Journal of cardiovascular computed tomography*. 2017 Jan 1;11(1):74-84. <https://doi.org/10.1016/j.jcct.2016.11.003>
  34. Hoori A, Al-Kindi S, Hu T, Song Y, Wu H, Lee J, Tashtish N, Fu P, Gilkeson R, Rajagopalan S, Wilson DL. Enhancing cardiovascular risk prediction through AI-enabled calcium-omics. *Scientific Reports*. 2024 May 15;14(1):11134. <https://doi.org/10.1038/s41598-024-60584-8>
  35. Rogers, M.A.; Aikawa, E. Cardiovascular calcification: Artificial intelligence and big data accelerate mechanistic discovery. *Nat. Rev. Cardiol*. 2019, 16, 261–274.
  36. Lim, L.J.; Tison, G.H.; Delling, F.N. Artificial Intelligence in Cardiovascular Imaging. *Methodist Debakey Cardiovasc. J*. 2020, 16,138–145.

42. Rubin, D.L. Artificial Intelligence in Imaging: The Radiologist's Role. *J. Am. Coll. Radiol.* 2019, 16, 1309–1317.
43. Abdelrahman, K.; Shiyovich, A.; Huck, D.M.; Berman, A.N.; Weber, B.; Gupta, S.; Cardoso, R.; Blankstein, R. Artificial Intelligence in Coronary Artery Calcium Scoring Detection and Quantification. *Diagnostics* 2024, 14, 125.
44. Wang W, Wang H, Chen Q, Zhou Z, Wang R, Wang H, Zhang N, Chen Y, Sun Z, Xu L.
45. Coronary artery calcium score quantification using a deep-learning algorithm. *Clin Radiol.*
46. 2020 Mar;75(3):237.e11-237.e16. doi: 10.1016/j.crad.2019.10.012. Epub 2019 Nov 11. PMID: 31718789. <https://doi.org/10.1016/j.crad.2019.10.012>
47. David J Winkel, V Reddappagari Suryanarayana, A Mohamed Ali, Johannes Görlich, Sebastian Johannes Buß, Axel Mendoza, Chris Schwemmer, Puneet Sharma, U Joseph Schoepf, Saikiran Rapaka, Deep learning for vessel-specific coronary artery calcium scoring: validation on a multi-centre dataset, *European Heart Journal - Cardiovascular Imaging*, Volume 23, Issue 6,
48. June 2022, Pages 846–854, <https://doi.org/10.1093/ehjci/jeab119>
49. Rana N, Sharma K, Sharma A. Diagnostic Strategies Using AI and ML in Cardiovascular Diseases: Challenges. *Deep Learning and Computer Vision: Models and Biomedical Applications: Volume 1.*:135. <https://doi.org/10.1007/978-981-96-1285-7>
50. Vivekanandan DD, Singh N, Robaczewski M, Wyer A, Canaan LN, Whitson D, Grabill N, Louis M. Artificial Intelligence-Driven Advances in Coronary Calcium Scoring: Expanding Preventive Cardiology. *Cureus.* 2024 Nov 28;16(11). <https://doi.org/10.7759/cureus.74681>
51. Onnis C, van Assen M, Muscogiuri E, Muscogiuri G, Gershon G, Saba L, De Cecco CN. The
52. Role of Artificial Intelligence in Cardiac Imaging. *Radiologic Clinics.* 2024 May 1;62(3):473-
53. 88. <https://doi.org/10.1016/j.rcl.2024.01.002>
54. Tolu-Akinnawo OZ, Ezekwueme F, Omolayo O, Batheja S, Awoyemi T. Advancements in Artificial Intelligence in Noninvasive Cardiac Imaging: A Comprehensive Review. *Clinical Cardiology.* 2025 Jan;48(1):e70087. <https://doi.org/10.1002/clc.70087>
55. Covas P, De Guzman E, Barrows I, Bradley AJ, Choi BG, Krepp JM, Lewis JF, Katz R, Tracy CM, Zeman RK, Earls JP. Artificial intelligence advancements in the cardiovascular imaging of coronary atherosclerosis. *Frontiers in cardiovascular medicine.* 2022 Mar 21;9:839400. <https://doi.org/10.3389/fcvm.2022.839400>
56. Gennari AG, Rossi A, De Cecco CN, van Assen M, Sartoretti T, Giannopoulos AA, Schwyzer M, Huellner MW, Messerli M. Artificial intelligence in coronary artery calcium score: rationale, different approaches, and outcomes. *The international journal of cardiovascular imaging.* 2024 May;40(5):951-66. <https://doi.org/10.1007/s10554-024-03080-4>
57. Yamaoka T, Watanabe S. Artificial intelligence in coronary artery calcium measurement: Barriers and solutions for implementation into daily practice. *European Journal of Radiology.* 2023 Jul 1;164:110855. <https://doi.org/10.1016/j.ejrad.2023.110855>
58. Eng D, Chute C, Khandwala N, Rajpurkar P, Long J, Shleifer S, Khalaf MH, Sandhu AT, Rodriguez F, Maron DJ, Seyyedi S. Automated coronary calcium scoring using deep learning with multicenter external validation. *NPJ digital medicine.* 2021 Jun 1;4(1):88.
59. Rumberger JA, Sheedy PF, Breen JF, Schwartz RS. Electron beam computed tomographic coronary calcium score cutpoints and severity of associated angiographic lumen stenosis. *Journal of the American College of Cardiology.* 1997 Jun;29(7):1542-8.
60. Rumberger JA, Brundage BH, Rader DJ, Kondos G. Electron beam computed tomographic coronary calcium scanning: a review and guidelines for use in asymptomatic persons. In *Mayo Clinic Proceedings* 1999 Mar 1 (Vol. 74, No. 3, pp. 243-252). Elsevier. <https://doi.org/10.4065/74.3.243>
61. Agatston AS, Janowitz WR, Hildner FJ, Zusmer NR, Viamonte M Jr, Detrano R. Quantification of coronary artery calcium using ultrafast computed tomography. *J Am Coll Cardiol* 1990; 15:827–832
62. Kulkarni S, Rumberger JA, Jha S. Electron beam CT: a historical review. *American Journal of Roentgenology.* 2021 May 24;216(5):1222-8. <https://doi.org/10.2214/AJR.19.22681>
63. El-Khoury GY, Bennett LD, Ondr GJ. Multidetector-row computed tomography. *JAAOS Journal of the American Academy of Orthopaedic Surgeons.* 2004 Jan 1;12(1):1-5.
64. Leschka, S., Scheffel, H., Desbiolles, L., Plass, A., Gaemperli, O., Stolzmann, P., ... Alkadhi, H. (2008). *Combining dual-source computed tomography coronary angiography and calcium scoring: added value for the assessment of coronary artery disease.* *Heart*, 94(9), 1154– 1161. <https://doi.org/10.1136/hrt.2007.124800>
65. Flohr TG, McCollough CH, Bruder H, Petersilka M, Gruber K, Süß C, Grasruck M,
66. Stierstorfer K, Krauss B, Raupach R, Primak AN. First performance evaluation of a dualsource CT (DSCT) system. *European radiology.* 2006 Feb;16:256-68. <https://doi.org/10.1007/s00330-005-2919-2>

67. George A, Movahed A. Coronary artery calcium scores: current thinking and clinical applications. The open cardiovascular medicine journal. 2008 Sep 18;2:87. <https://doi.org/10.2174/1874192400802010087>.

68. Wang L, Jerosch-Herold M, Jacobs DR, Shahar E, Detrano R, Folsom AR, MESA Study Investigators. Coronary artery calcification and myocardial perfusion in asymptomatic adults: the MESA (Multi-Ethnic Study of Atherosclerosis). Journal of the American College of Cardiology. 2006 Sep 5;48(5):1018-26. <https://dx.doi.org/10.1016/j.jacc.2006.04.089>

69. Majhi L. Revolutionizing Risk Assessment: Coronary Artery Calcium Score in Cardiovascular Disease Management. Disease management.;35(48):51.

70. <https://dx.doi.org/10.21275/SR24523083602>

**Table 1. Methods for Calculating CAC Score (Gupta, A et al., 2022).**

| Calcium scoring method  | Strengths  | Limitations   |
|---|--|---|
| <b>Agatston score</b><br><b>Score</b><br>(Calculated as plaque area × attenuation weighting factor) | Most extensively studied and commonly applied method; considered the reference standard- Straightforward postprocessing methodology  | Susceptible to fluctuations caused by minor image noise- Requires strict compliance with the original protocol for consistency- Exhibits limited reproducibility between repeated scans |
| <b>Volume score</b><br>(Calculated as plaque area × slice thickness)                                | Less influenced by minor variations in image noise- Simple and efficient postprocessing- Demonstrates improved reproducibility across serial scans   | Does not incorporate plaque attenuation into the calculation- Lower validation in clinical research compared to Agatston score  |
| <b>Mass score</b><br>(Calculated as plaque volume × calibration factor × mean plaque attenuation)   | Provides a more direct measurement of calcium hydroxyapatite content in the plaque- Demonstrates greater resistance to noise-related variability- Offers enhanced reproducibility in repeated examinations | Involves more complex and timeintensive postprocessing- Least validated method, with limited clinical data supporting its use   |

**Table 2. Clinical Application of Artificial Intelligence in Cardiac Imaging.(Abdelrahman et al., 2024)**

| Category                 | Clinical Application            | Description  | Clinical Advantage   |
|--------------------------|---------------------------------|--|--|
| <b>Image Acquisition</b> | <b>Radiation Dose Reduction</b> | Deep learning-based reconstruction algorithms simulate high-quality images from low-dose CT data | Preserves diagnostic image quality while significantly lowering radiation exposure to patients |
|                          | <b>CMR Plane Positioning</b>    | AI automatically identifies key anatomical landmarks for precise slice alignment                 | Produces standardized, reproducible, and diagnostically accurate imaging planes                |

|                           |                                       |   |  |
|---------------------------|---------------------------------------|---|--|
|                           | <b>CMR Acquisition Time Reduction</b> | DL accelerates cine sequence acquisition through undersampling and image reconstruction | Minimizes scan duration and number of breathholds, especially beneficial for pediatric or uncooperative patients |
| <b>Image Optimization</b> | <b>Denosing</b>                       | AI-driven models remove noise and correct motion artifacts from raw imaging datasets    | Improves clarity and accuracy of image interpretation across modalities  |
|                           | <b>Non-contrast Image Enhancement</b> | AI enhances soft tissue contrast and visibility in noncontrast images                   | Avoids the need for gadolinium or iodinebased contrast agents, reducing potential risks for renal patients       |
| <b>Outcome Prediction</b> | <b>MACE Risk Prediction</b>           | ML models synthesize clinical history,  | Enhances prediction accuracy beyond  |

|                                |   |  |   |
|--------------------------------|---|--|---|
|                                |   | laboratory data, and imaging biomarkers to assess MACE risk  | traditional risk models and facilitates early intervention                                  |
| <b>Coronary Artery Disease</b> | <b>Coronary Calcium Scoring</b>         | Automated or semiautomated CAC scoring from ECGgated and non-ECGgated CT   | Enables faster and reproducible risk stratification using widely accessible CT techniques   |
|                                | <b>Plaque Characterization</b>          | DL models classify atherosclerotic plaque types and detect highrisk features (e.g., low-attenuation, napkin-ring sign) | Reduces manual evaluation time and supports early identification of vulnerable plaques      |
|                                | <b>CT-derived FFR (CT-FFR)</b>          | ML calculates fractional flow reserve using coronary CT angiography without invasive procedures                        | Offers functional assessment of stenosis severity with reduced cost, time, and patient risk |
|                                | <b>Epicardial Fat Quantification</b>    | AI segments and quantifies pericoronary and epicardial adipose tissue  | Provides novel markers for cardiovascular risk, with reduced manual workload                |
|                                | <b>Myocardial Infarction Assessment</b> | AI detects and segments infarcted regions on noncontrast CMR sequences   | Eliminates contrast use, improves workflow, and enhances prognostic accuracy                |

|                                       |  |  |  |
|---------------------------------------|--|--|--|
| <b>Myocardial Function</b>            | <b>Volume Analysis</b>                           | AI automatically segments ventricular cavities for calculating ejection fraction, EDV, and ESV             | Saves time, standardizes measurements, and reduces inter-observer variability                      |
|                                       | <b>Myocardial Strain Measurement</b>             | AI quantifies strain from cine or tagged MR images, eliminating need for dedicated sequences               | Increases adoption and diagnostic depth of strain imaging, even in routine settings                |
| <b>Valvular Heart Disease</b>         | <b>AI-Based Classification</b>                   | AI assesses and grades severity of valvular dysfunction from flow velocity and regurgitation data          | Streamlines diagnosis, reduces reporting time, and supports early intervention planning            |
| <b>Cardiomyopathies</b>               | <b>Disease Classification and LGE Evaluation</b> | AI detects hypertrophic, dilated, or restrictive patterns, and evaluates late gadolinium enhancement (LGE) | Improves diagnostic precision and supports long-term prognosis evaluation                          |
| <b>Congenital Heart Disease (CHD)</b> | <b>Image Acquisition &amp; Reconstruction</b>    | AI-assisted protocols optimize acquisition of high-resolution images tailored for complex CHD anatomy      | Enhances image quality and reduces scanning/postprocessing time, critical in pediatric populations |

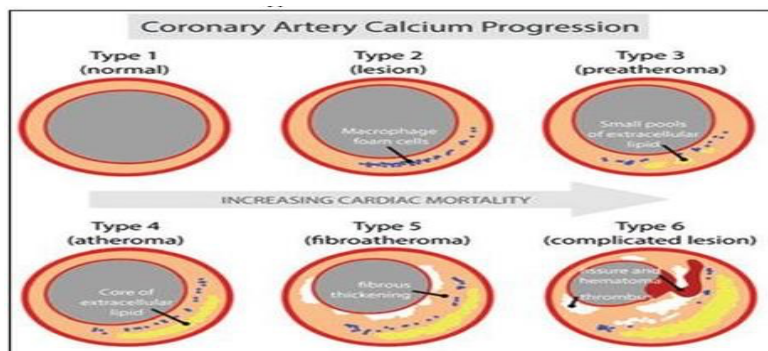
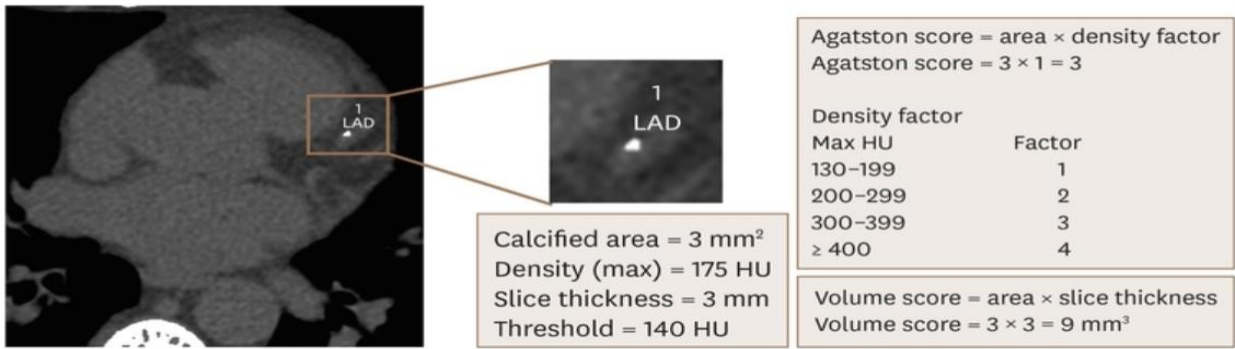


Figure 1 : Pathophysiology of coronary artery calcification progression (Quddus R et al., 2024)

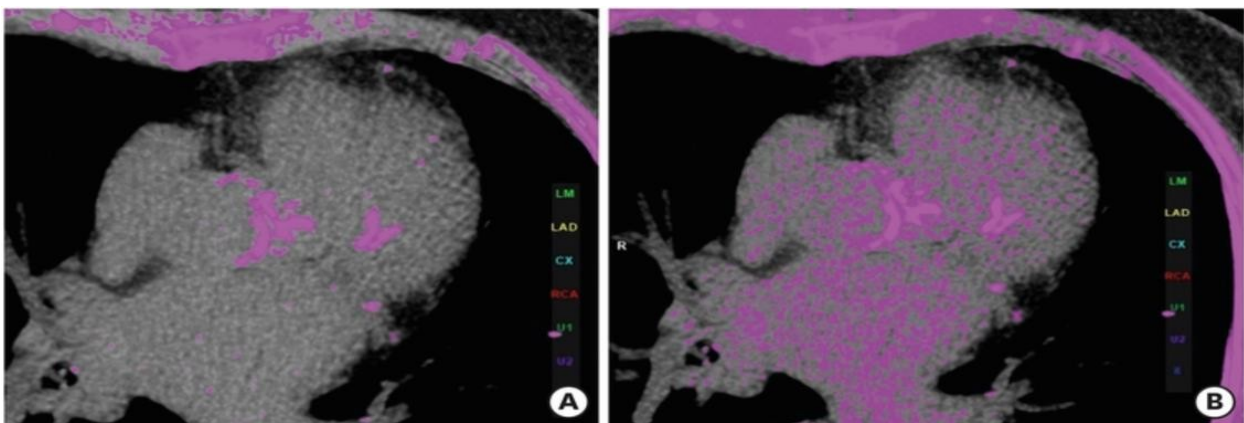


Figure 2: Example of Agatston and volume score calculation. The illustration displays a single 3 mm<sup>2</sup> calcified plaque with a maximum CT number of 175 HU. The area of the lesion is multiplied by the




**Figure 3 :** Calcium score for the heart. (A) A non-contrast ECG gated axial CT scan of the coronary arteries shows that the anatomic region of the proximal segments of the left circumflex (blue) coronary arteries, the proximal segment of the RCA (red), and its branch has several calcified plaque. The aortic

density factor to determine the Agatston score. Predetermined cutoff values are used to calculate the density factor. The calculated area multiplied by slice thickness yields the volume score. The final result is produced by adding the scores for each individual lesion. (Kumar P et al., 2023) root's calcification are shown by the white spots. (B) The CT workstation's measurement table shows each coronary artery's Agatston, volume, and mass calcium scores as well as the overall score. 130 HU is the cutoff point for determining the Agatston score. 0.81 is the mass calibration factor. (Kumar P et al., 2023)




**Figure 4 :** Shows how the CT threshold affects the computation of the CAC score. The threshold is set at 130 HU in (A) and 110 HU in (B). Image noise significantly increases when the threshold is lowered by 20 HU, which may change the final score. (Kumar P et al., 2023)

**Figure 5 :** Moving Beyond the Agatston Score (Blaha, M.J. et al., 2017).

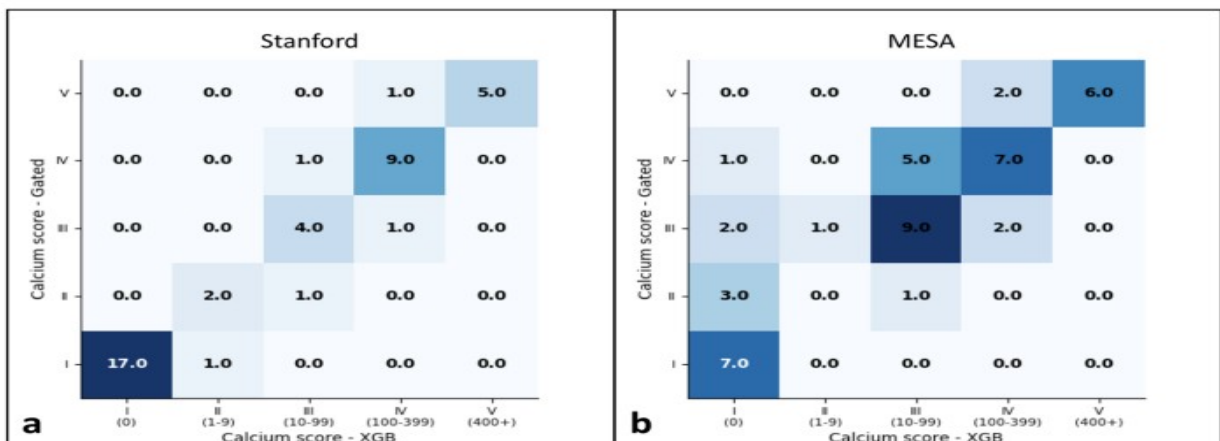

**Figure 6 :** Internal and MESA datasets are used to compare automated and manual CAC grading on non-gated chest CT exams. Confusion matrices comparing automated scoring of non-gated chest CT tests to ground truth scores for the Stanford (a) and MESA (b) test sets. In each matrix, the x-axis represents the model prediction and the y-axis represents the ground truth scores. (Eng D et al., 2021)

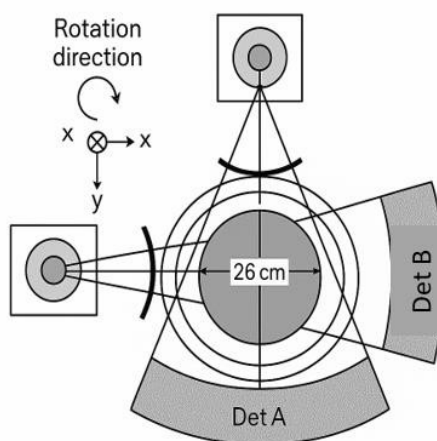

**Figure 7.** Dual-source computed tomography (DSCT) system engineering and implementation. With a diameter of 50 cm, one detector (A) cover the whole scan field of view, but due to gantry space

constraints, the other detector (B) is only able to cover a narrow, center field of view.( Flohr TG et al., 2006)

Contact information

**Ms. Shipra Saroj, Assistant Professor, Department of Paramedical Science, Institute-Rayat Bahra University Punjab, 140413, [shiprasaroj789@gmail.com](mailto:shiprasaroj789@gmail.com), +91 7393059543**

**Sohel Rana, Assistant Professor, Department of Paramedical Science, Midnapore City College, Midnapore, 721129, [sohelrana9831@gmail.com](mailto:sohelrana9831@gmail.com), +91 9831716187**